



**NOTE:**  
GAS ANALYZER REQUIRES 14 INCHES OF CLEARANCE FOR DOOR SWING.

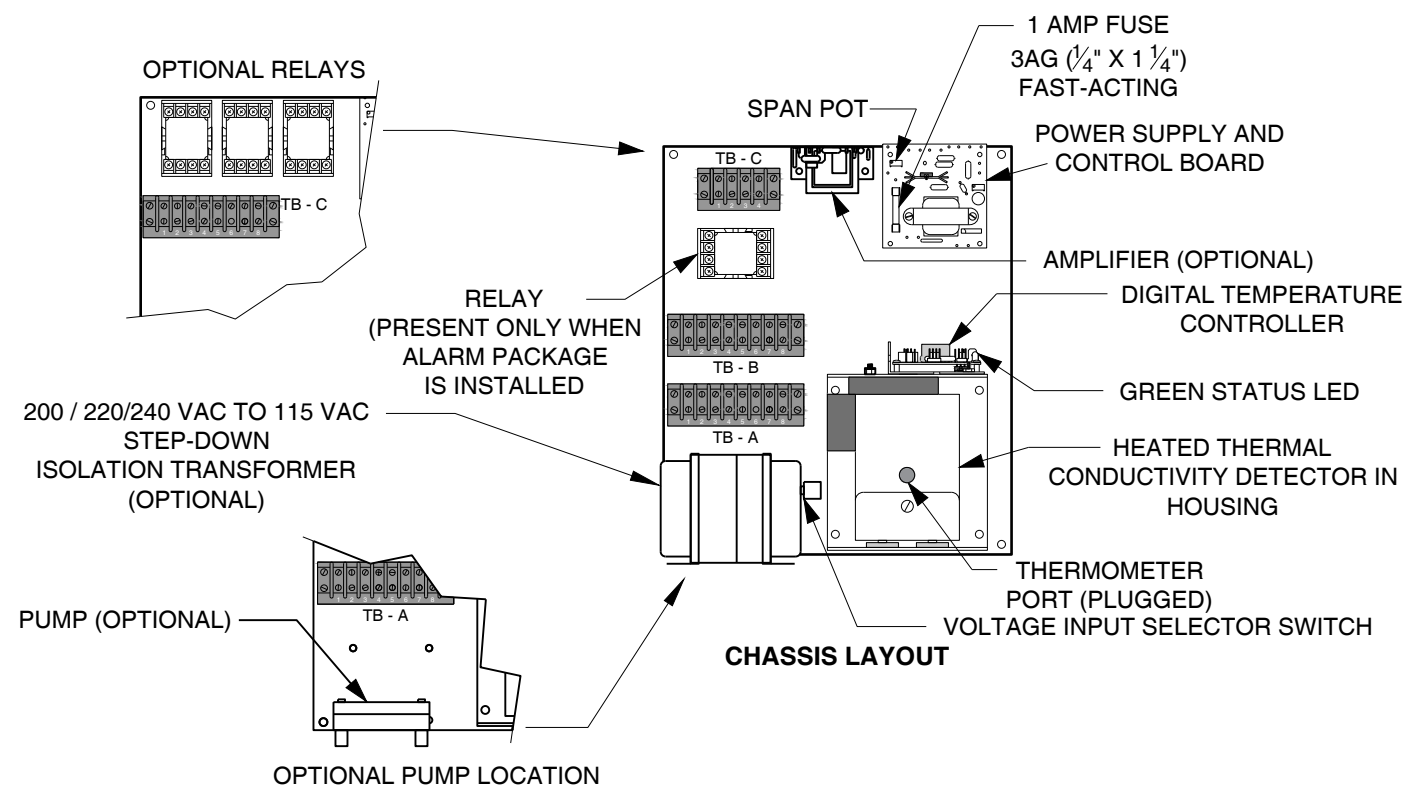

STEP-DOWN TRANSFORMER VOLTAGE INPUT SELECTOR SWITCH SETTINGS

DO NOT ADJUST THIS SETTING UNLESS YOU HAVE CONSULTED WITH THE FACTORY

NOMINAL AC INPUT VOLTAGE	INPUT SELECTOR SWITCH SETTING
200	210
220	230
240	250

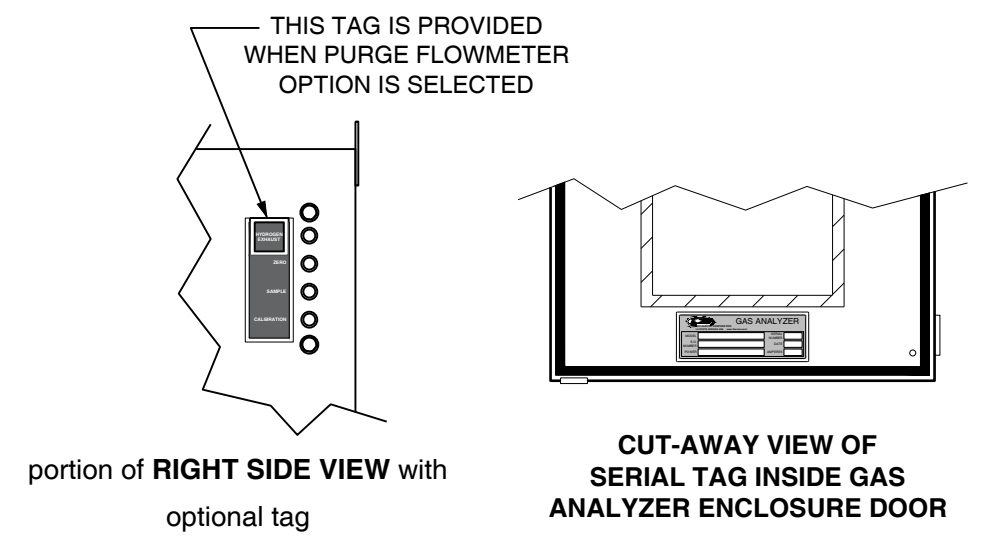

**NOTES:**

- ALL DIMENSIONS ARE IN INCHES UNLESS OTHERWISE INDICATED.
- REFER TO DATA SHEET TO DETERMINE WHICH OPTIONS ARE PRESENT.

H			
G			
F			
E			
D			
C			
B			
A	GRAPHICAL UPDATES; ADDED SAMPLE PORT NOTE	GAR	9-3-20
REVISIONS		BY	DATE

**Thermco** INSTRUMENT CORPORATION  
LA PORTE, INDIANA USA

TITLE: **INSTRUCTION DRAWING FOR MODEL 7010 GAS ANALYZER**

DATE: 9-9-20  
SCALE: N.T.S.  
DRAWN BY: JTM  
APPROVED BY: GAR  
SUPERSEDES: 2-13244  
DRAWING NUMBER: 2-14591